


Open Quartz Cell with a Tube

MQQLW005 | Features and requirements to define

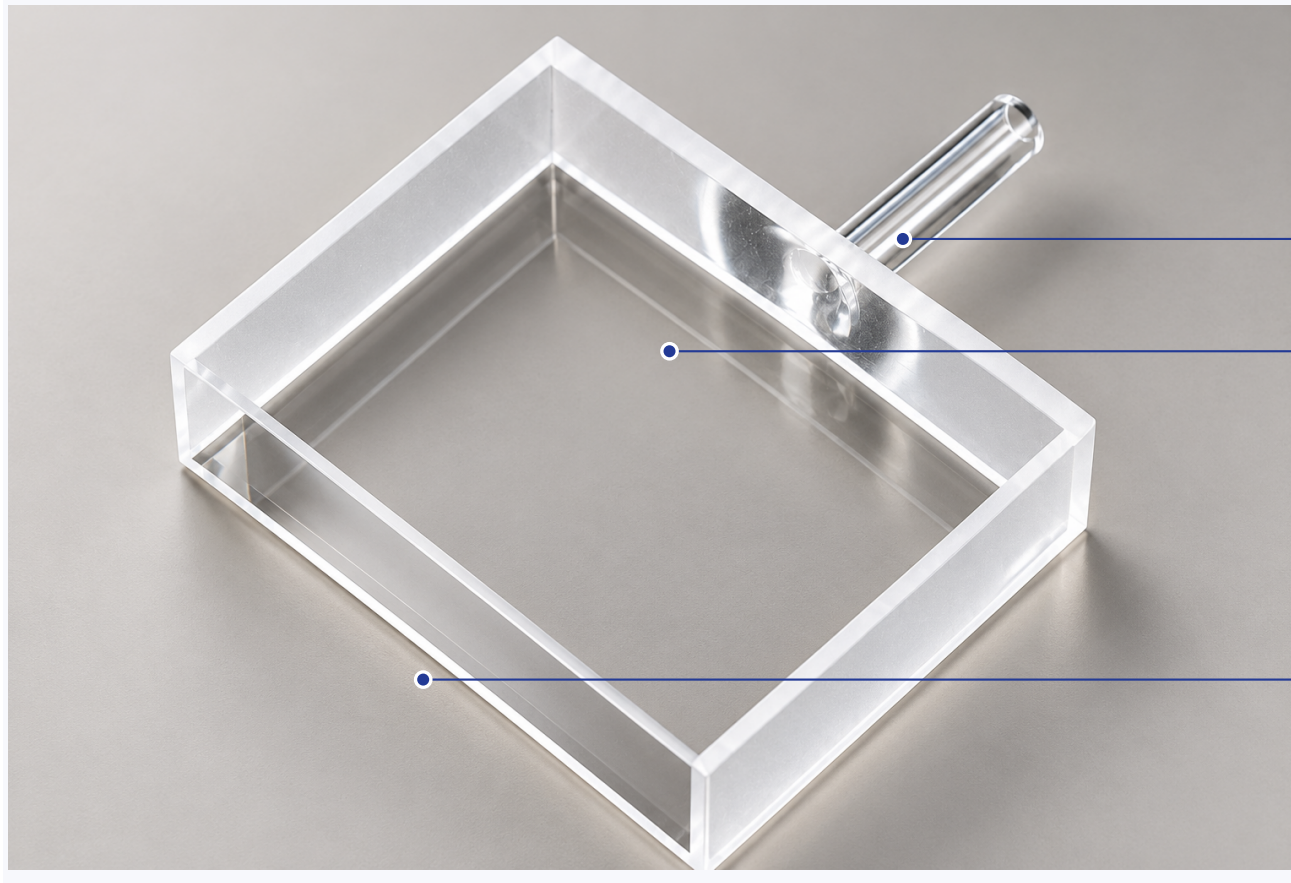

1 Single connection feature

Define the role of the single projecting tube.

2 Open-mouth access

Keep the large open mouth accessible.

3 Installed support datum

Locate the body from an agreed support datum.

REFERENCE VALUES

Nominal path

10 mm

Nominal capacity

17.5 mL

Illustrative design example; not an actual customer requirement.

Not to scale. Product-reference rendering with annotations; use the agreed drawing for dimensional acceptance.